

Appendix C. Graphical Presentations

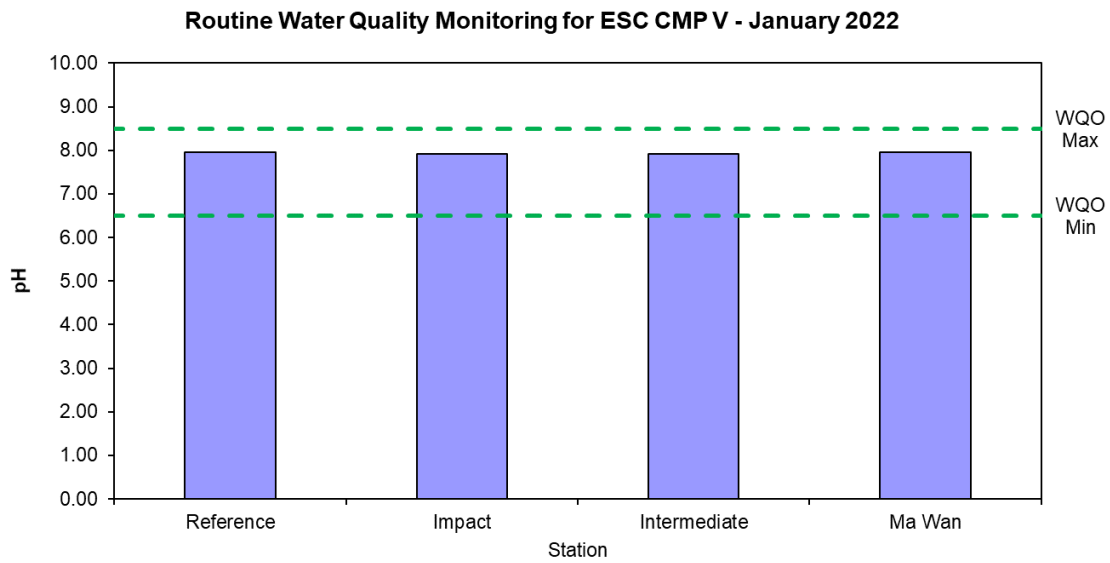


Figure 1: Level of pH recorded during Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

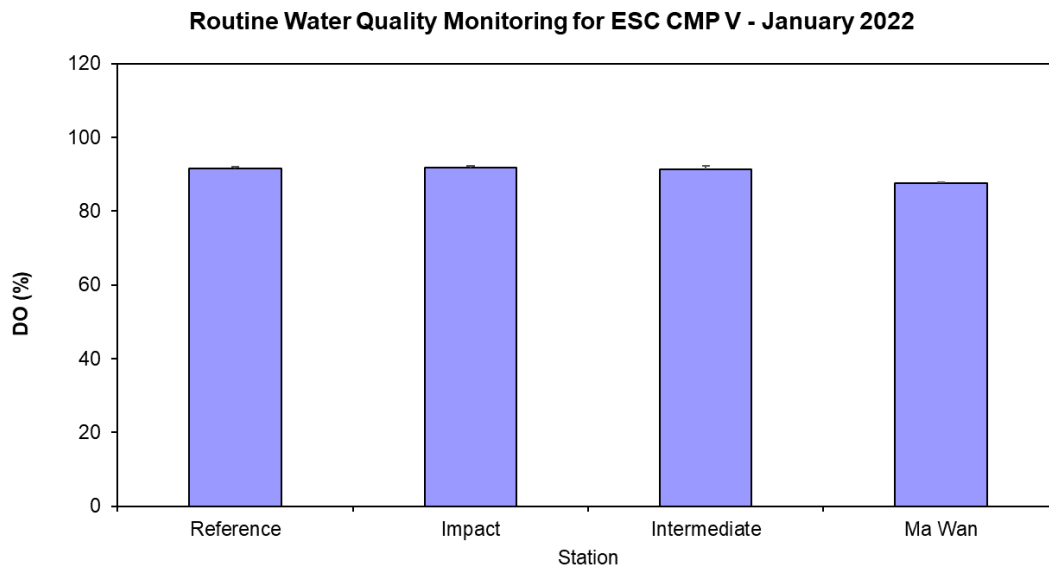


Figure 2: Level of Dissolved Oxygen (DO) (% saturation; mean + SD)¹ recorded during Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

¹ The mean and standard deviation (SD) for in-situ data are the mean and SD for water columns within the area.

Routine Water Quality Monitoring for ESC CMP V - January 2022

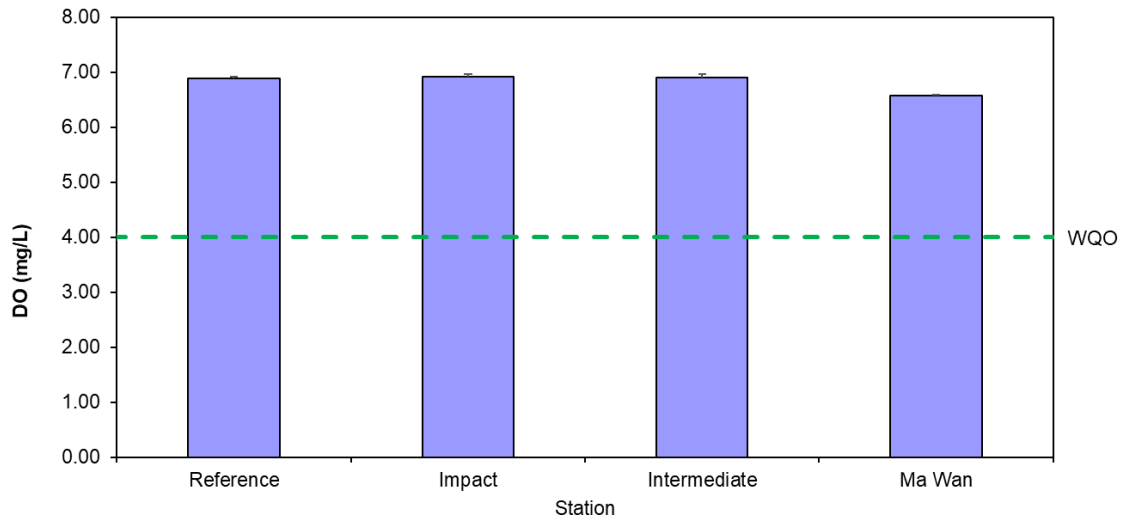


Figure 3: Concentration of Dissolved Oxygen (DO) (mg/L; mean + SD)¹ recorded during Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

Routine Water Quality Monitoring for ESC CMP V - January 2022

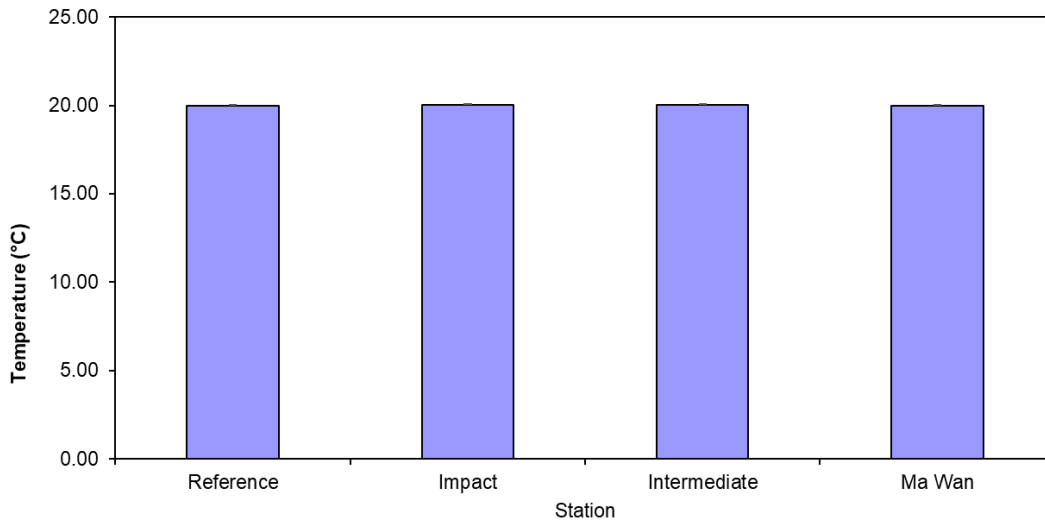


Figure 4: Level of Temperature (°C; mean + SD)¹ recorded during Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

¹ The mean and standard deviation (SD) for in-situ data are the mean and SD for water columns within the area.

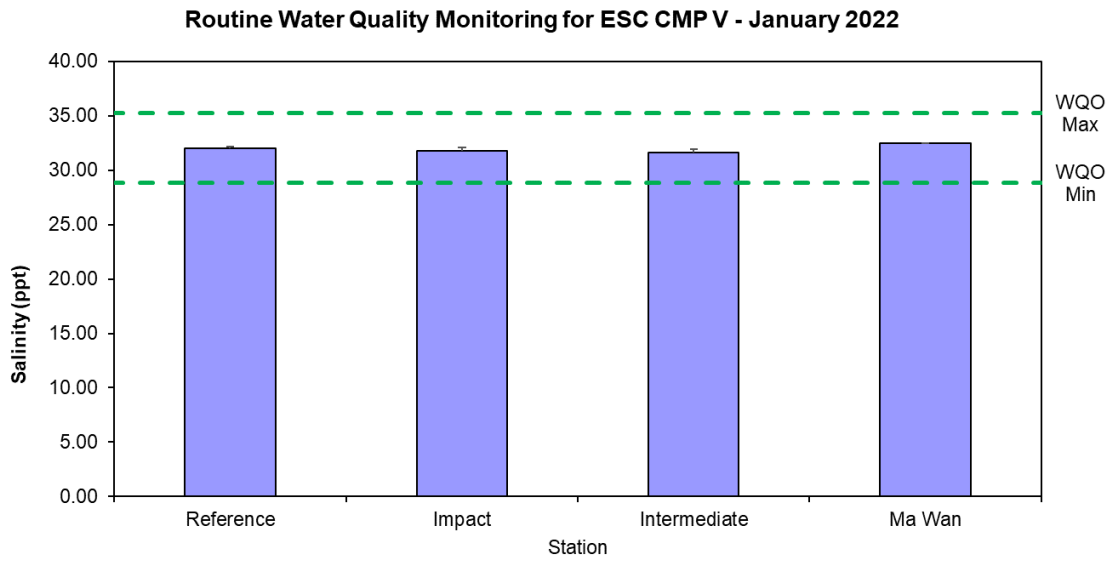


Figure 5: Level of Salinity (ppt; mean + SD)¹ recorded during Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

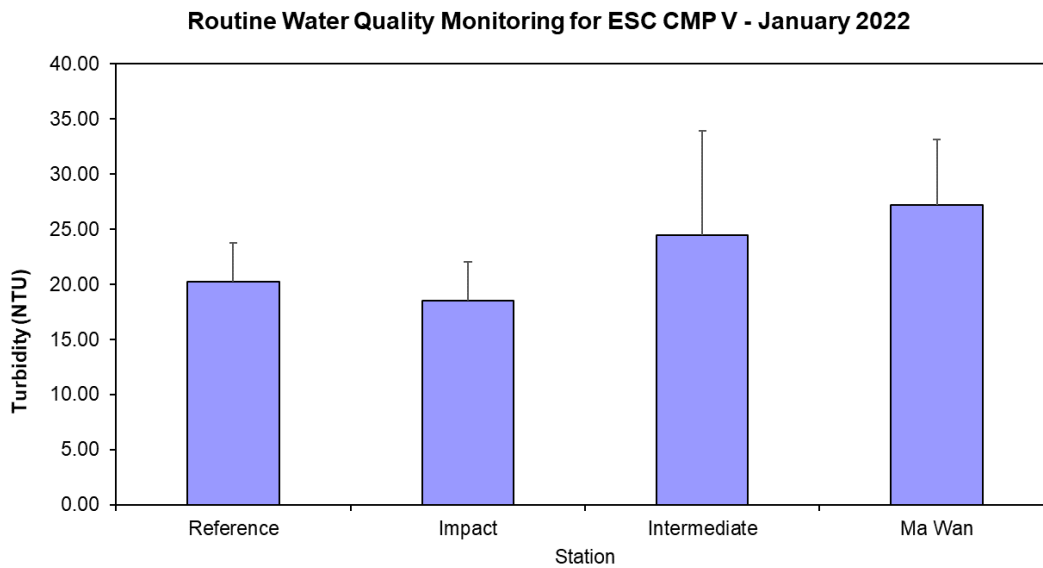


Figure 6: Level of Turbidity (NTU; mean + SD)¹ recorded during Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

¹ The mean and standard deviation (SD) for in-situ data are the mean and SD for water columns within the area.

Routine Water Quality Monitoring for ESC CMP V January 2022

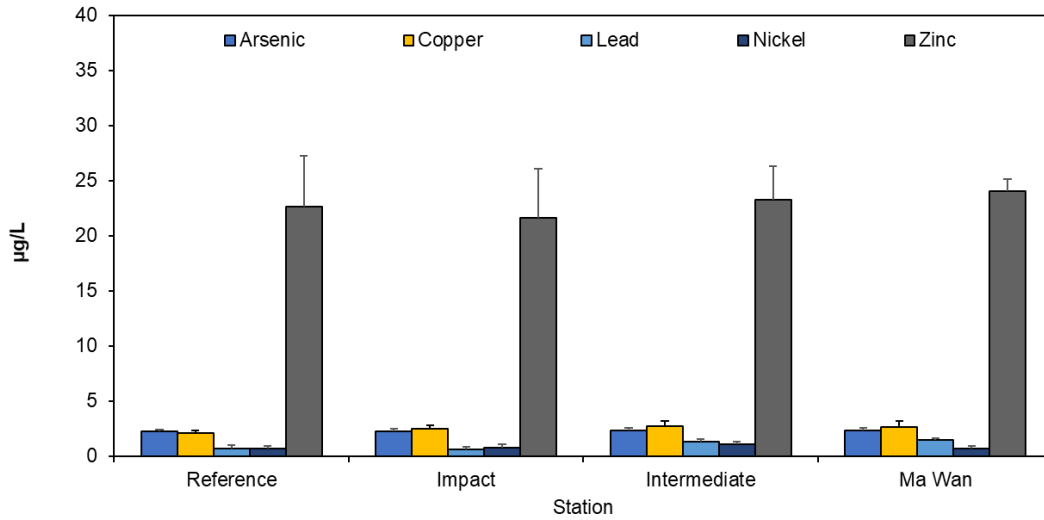


Figure 7: Concentration of Arsenic, Copper, Lead, Nickel, and Zinc (µg/L; mean + SD) in water samples collected from Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

Routine Water Quality Monitoring for Nutrients - January 2022

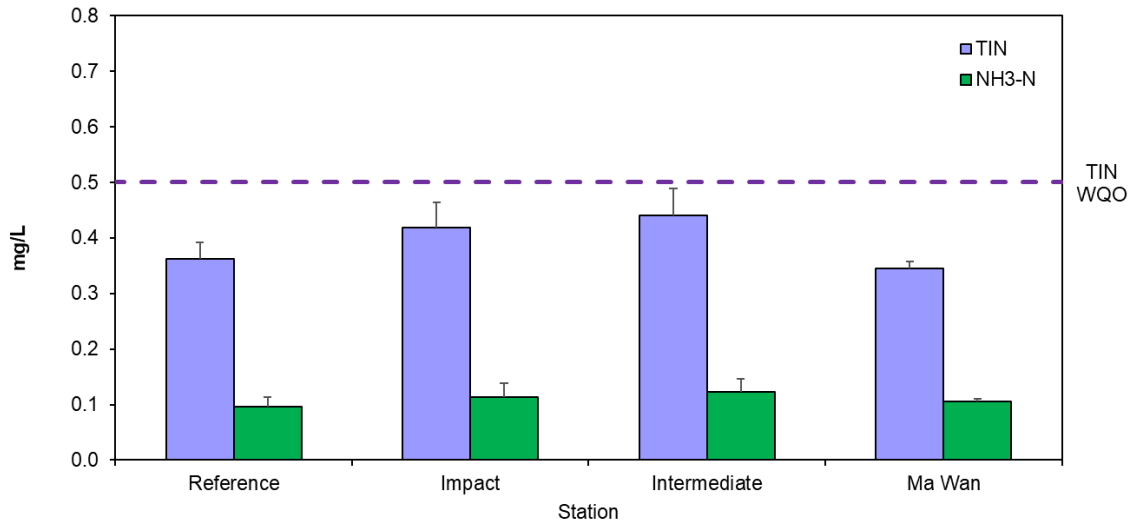


Figure 8: Concentration of Total Inorganic Nitrogen (TIN) and Ammonia Nitrogen (NH3-N) (mg/L; mean + SD) in water samples collected from Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

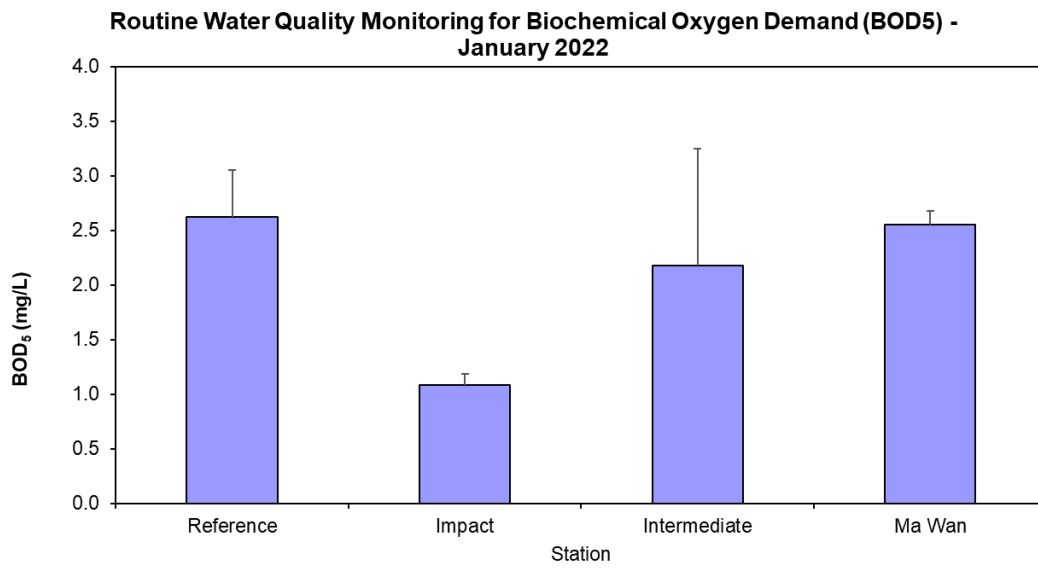


Figure 9: Level of Biochemical Oxygen Demand (BOD₅) (mg/L; mean + SD) in water samples collected from Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

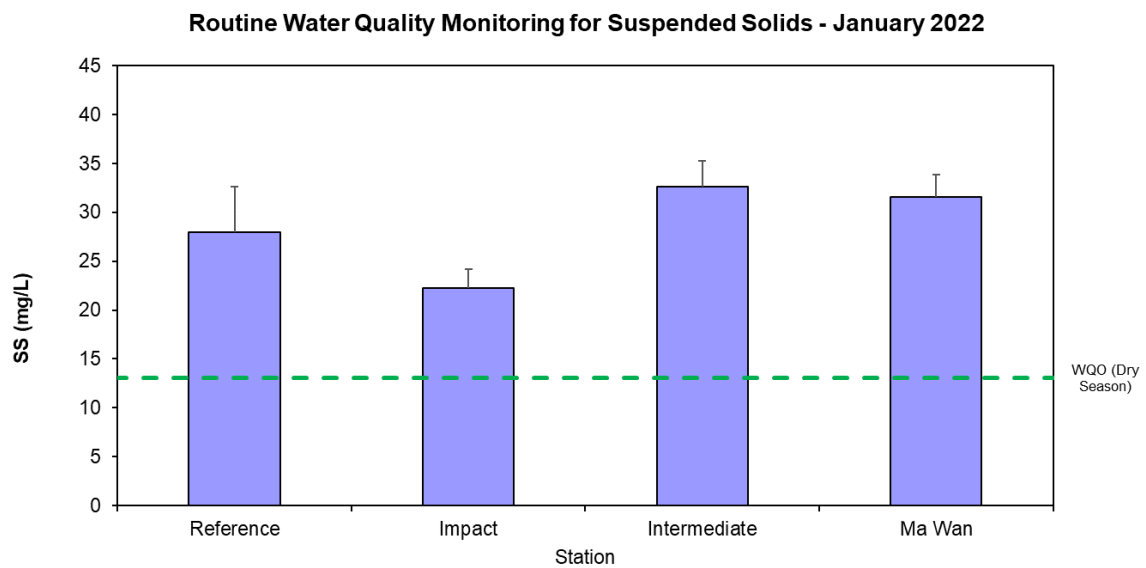


Figure 10: Concentration of Suspended Solids (SS) (mg/L; mean + SD) in water samples collected from Routine Water Quality Monitoring for disposal operations at ESC CMP V in January 2022

Pit Specific Sediment Chemistry for Metal and Metalloid Contaminants at ESC CMP Vb - January 2022

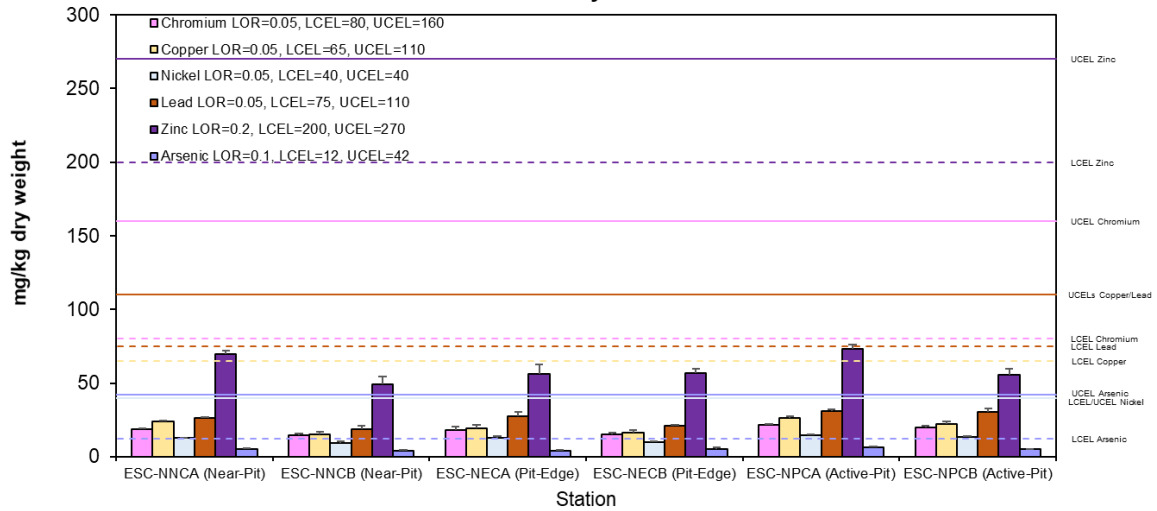


Figure 11: Concentration of Metals and Metalloid (Cr, Cu, Ni, Pb, Zn, As; mg/kg dry weight; mean + SD) in sediment samples collected from Pit Specific Sediment Chemistry Monitoring for ESC CMP Vb in January 2022

Pit Specific Sediment Chemistry for Metal Contaminants at ESC CMP Vb - January 2022

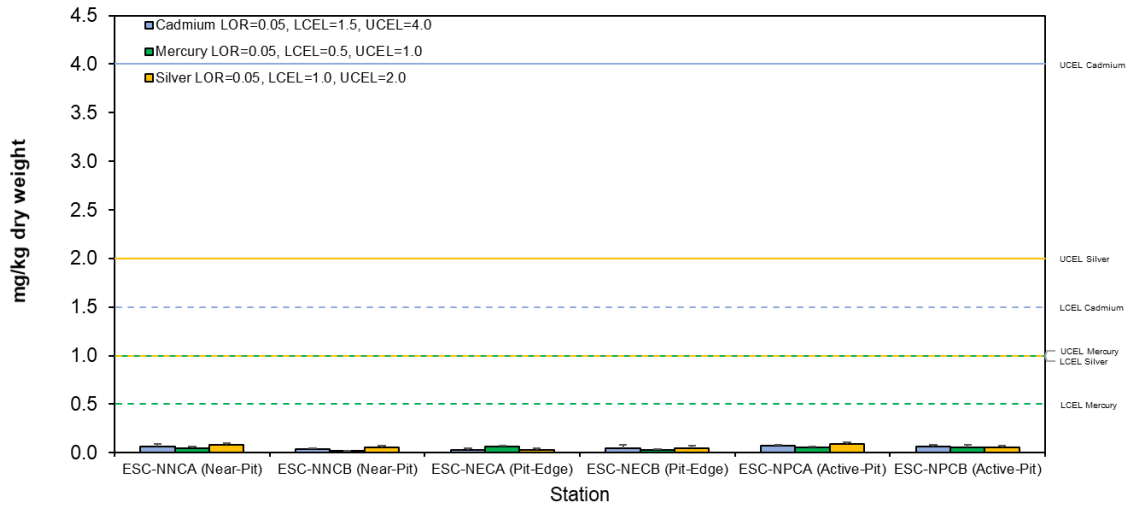


Figure 12: Concentration of Metals (Cd, Hg, Ag; mg/kg dry weight; mean + SD) in sediment samples collected from Pit Specific Sediment Chemistry Monitoring for ESC CMP Vb in January 2022

Pit Specific Sediment Chemistry for Total Organic Carbon (TOC) at ESC CMP Vb - January 2022

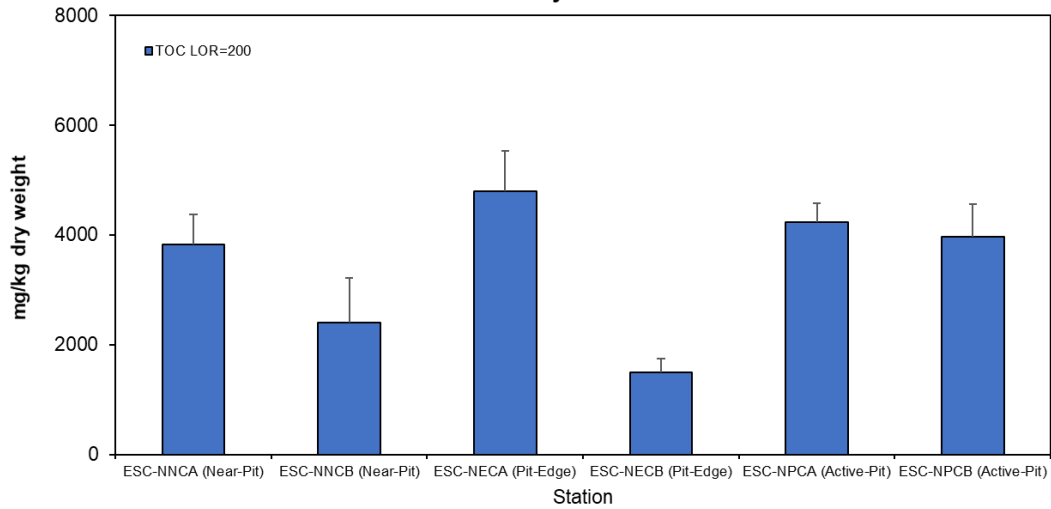


Figure 13: Concentration of Total Organic Carbon (TOC) (mg/kg dry weight; mean + SD) in sediment samples collected from Pit Specific Sediment Chemistry Monitoring for ESC CMP Vb in January 2022

Pit Specific Sediment Chemistry for Low and High Molecular Weight Polycyclic Aromatics Hydrocarbons (PAHs) at ESC CMP Vb - January 2022

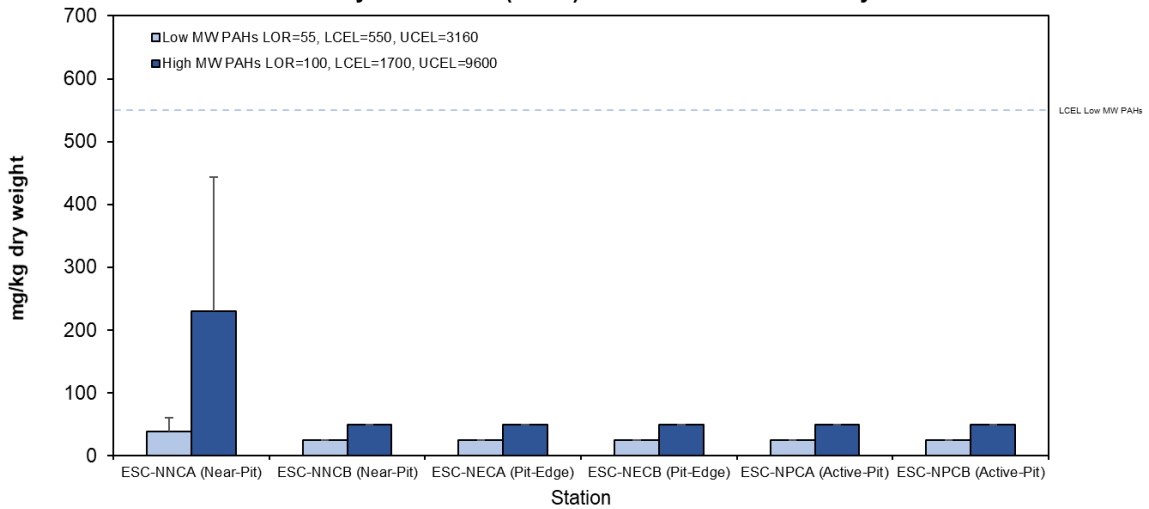


Figure 14: Concentration of Low and High Molecular Weight Polycyclic Aromatic Hydrocarbons (mg/kg dry weight; mean + SD) in sediment samples collected from Pit Specific Sediment Chemistry Monitoring for ESC CMP Vb in January 2022

Pit Specific Sediment Chemistry for Tributyltin (TBT) at ESC CMP Vb - January 2022

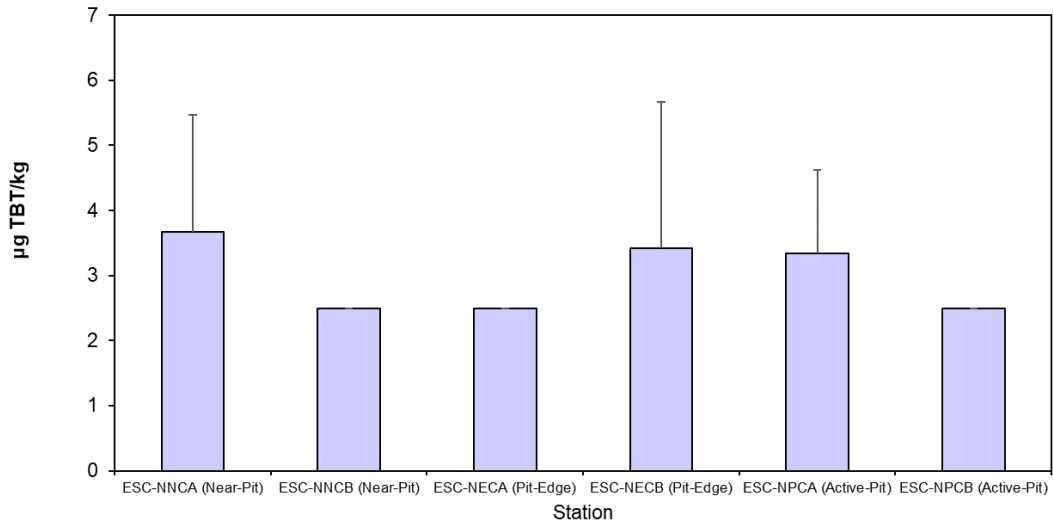


Figure 15: Concentration of Tributyltin (TBT) ($\mu\text{g TBT/kg}$; mean + SD) in sediment samples collected from Pit Specific Sediment Chemistry Monitoring for ESC CMP Vb in January 2022